

HEAD CTA ANEURYSM PHANTOM

Age
Category

Adult

Body
Region

Head

Target
Modality

CT

Diagnostic
Features

Brain aneurysms




This phantom simulates a contrast medium enhanced head in arterial phase (CT angiography). It covers the vertex to the foramen magnum.


The phantom has three intracranial aneurysms of the middle cerebral artery (MCA), anterior communicating artery (ACoA), and the basilar artery.

The phantom can be used in CT (including CBCT) to evaluate and optimize imaging performance and AI-enabled diagnosis. It is also suited for training purposes.

The phantom provides a detailed and realistic simulation of common brain pathologies, soft and bone tissues. Air voids are filled with a cellulose-polymer composite of approx. -160 HU.

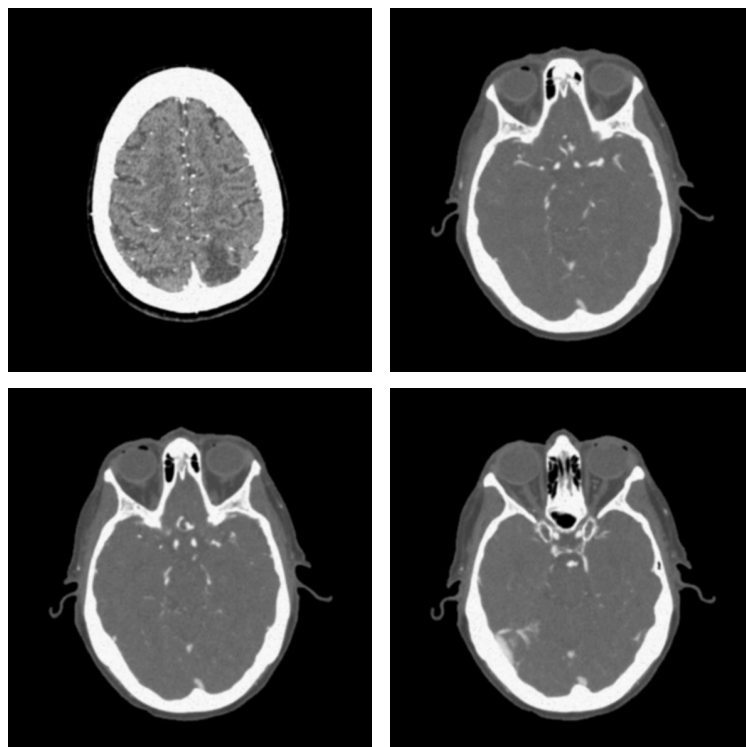

HEAD CTA ANEURYSM PHANTOM

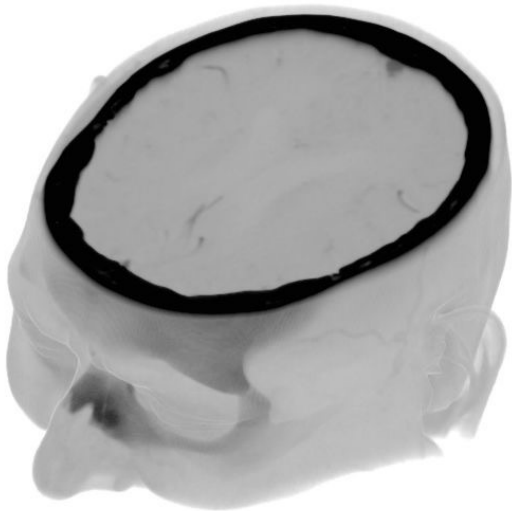

Specifications


Size	Approx. 191 x 218 x 150 mm 7.5 x 8.6 x 5.9 in
Weight	Approx. 2680 g 5.9 lb
Base material	Cellulose-polymer composite
Optimal tube voltage	120 kVp (cf page 5) - adaptable upon request -

Diagnostic features

Realistic simulation of head vessels, bone and soft tissues.


Aneurysms:

- Middle cerebral artery (MCA)
left side
- Anterior communicating artery (ACoA)
left side
- Basilar artery
left side


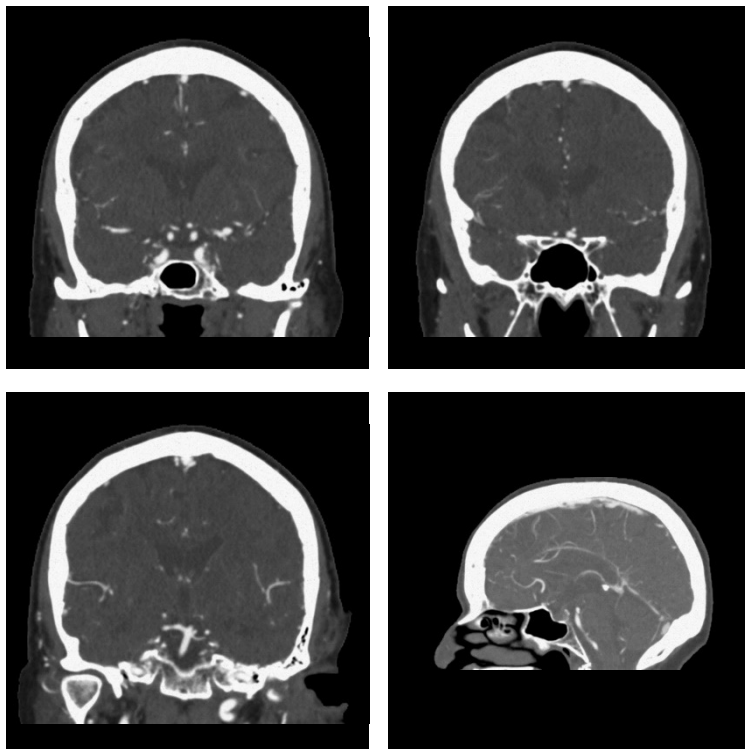


For more information visit
www.phantomx.de

HEAD CTA ANEURYSM PHANTOM


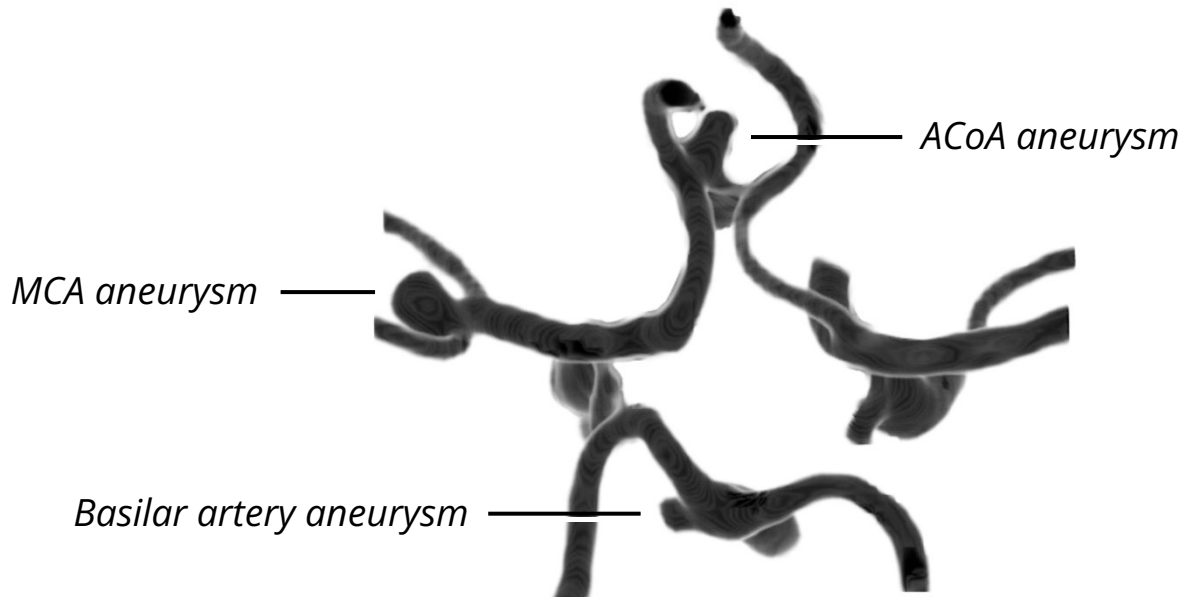


Middle cerebral artery (MCA) aneurysm (left side)

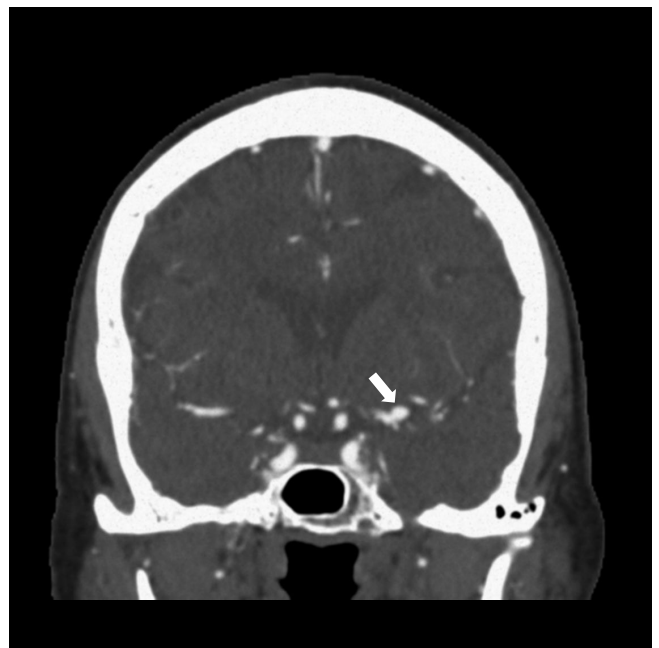
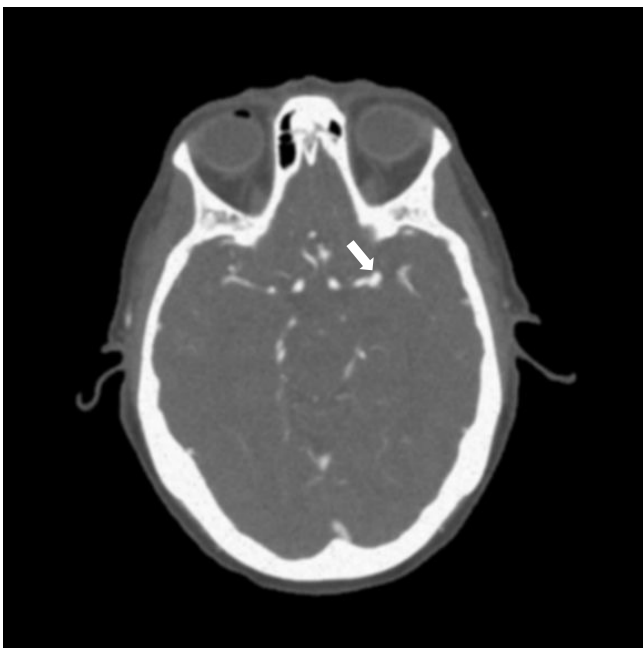


HEAD CTA ANEURYSM PHANTOM

Anterior communicating artery (ACoA) aneurysm (left side)

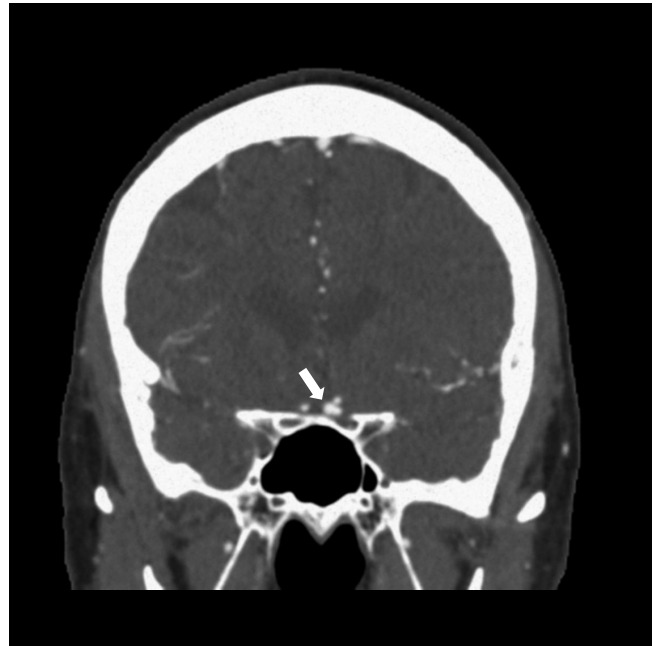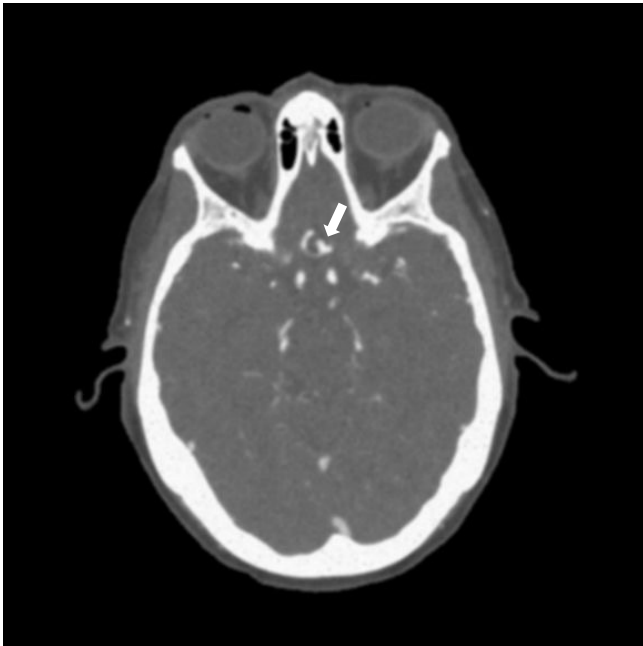

Basilar artery aneurysm (left side)

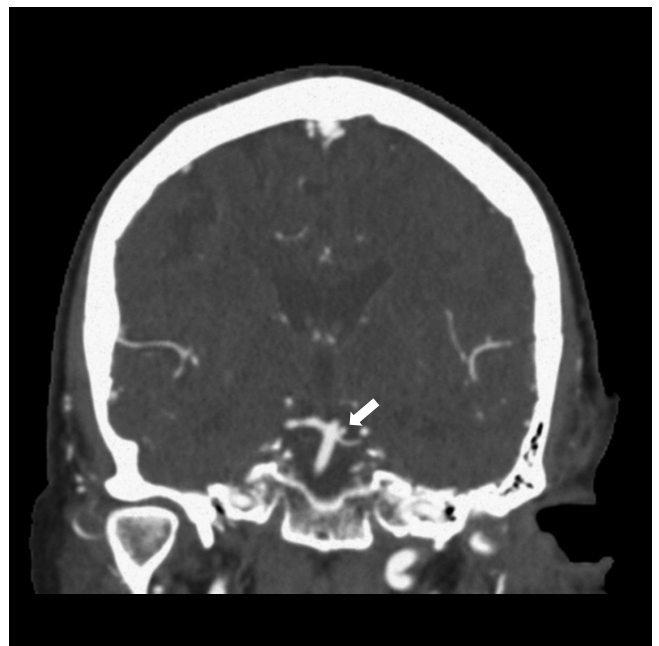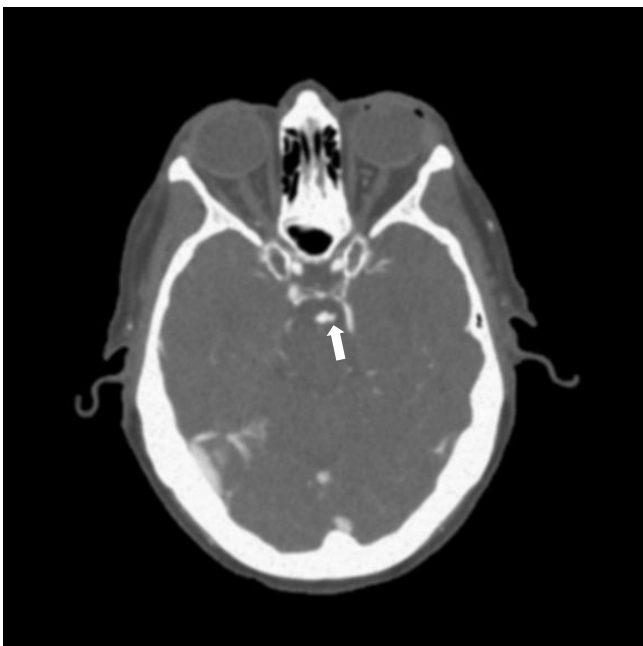

HEAD CTA ANEURYSM PHANTOM


General indications

- The phantom is made of a cellulose-polymer composite material with properties similar to hardwood. If handled carefully, it will last a long time.
- The phantom is coated with a protective layer. If the protective layer is undamaged, the phantom can be cleaned using a damp cloth (water or mild detergent).
- Protect from direct sunlight.
- Maintain a storage temperature of 10 °C to 30 °C. If the phantom is exposed to temperatures below -10 °C or above 45 °C, it can be severely damaged.
- The phantom is not equipped for dose measurements with dosimeters and it is not suited for material characterization with dual energy CT.
- The phantom is not certified as medical device.
- Air voids are filled with cellulose-polymer composite of approx. -160 HU.
- Handle with care to prevent injury or damage.
- If external damage is observed, it is recommended to consult PhantomX.


Attenuation properties

Soft Tissue

Linear attenuation coefficients [cm^{-1}] (calculated)

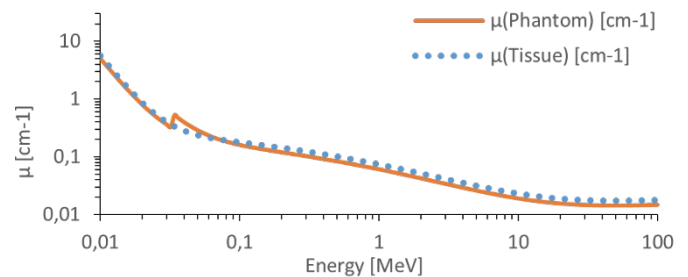


Hounsfield units (calculated)

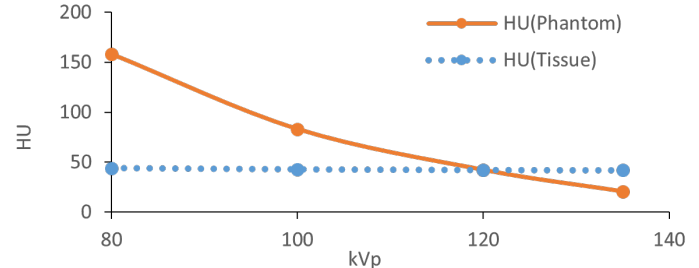


Bone Tissue

Linear attenuation coefficients [cm^{-1}] (calculated)

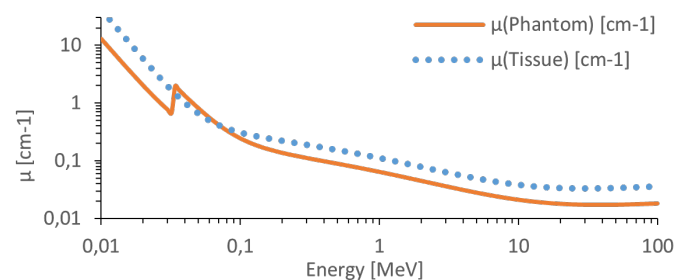

Hounsfield units (calculated)

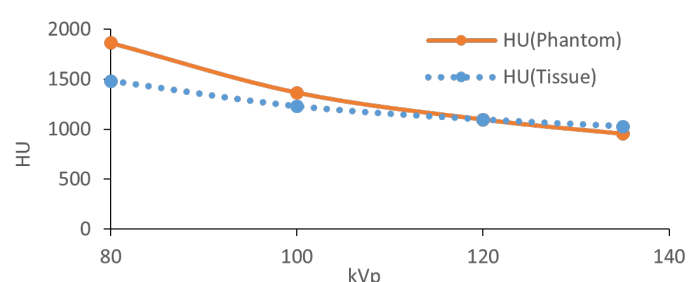

Tissue Reference: Woodard HQ, White DR. The composition of body tissues. Br J Radiol. 1986.