

# BREAST PHANTOM

Age  
Category

Adult

Body  
Region


Breast

Target  
Modality

Mammography,  
Tomosynthesis

Diagnostic  
Features

Masses,  
Calcifications

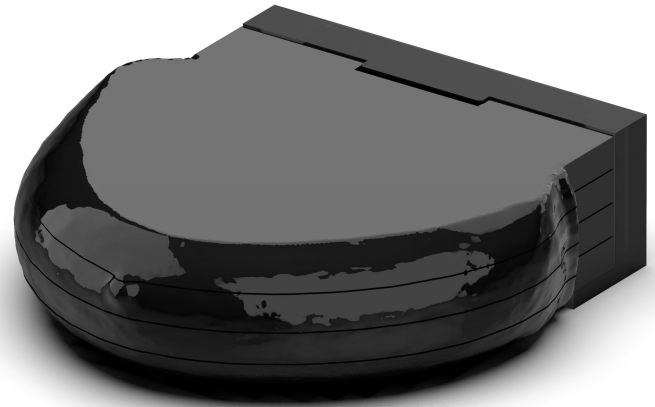


This phantom simulates a compressed breast. It is composed of four slabs that are held together by a magnetic mount.


The phantom can be equipped with an insertable pattern to simulate microcalcifications. The central slabs can be replaced to simulate a breast mass.

The phantom can be used in mammography and breast tomosynthesis to evaluate and optimize imaging performance and post-processing applications, including AI-enabled applications. It is also suited for training purposes.


The phantom provides a detailed and realistic simulation of glandular and adipose tissue.

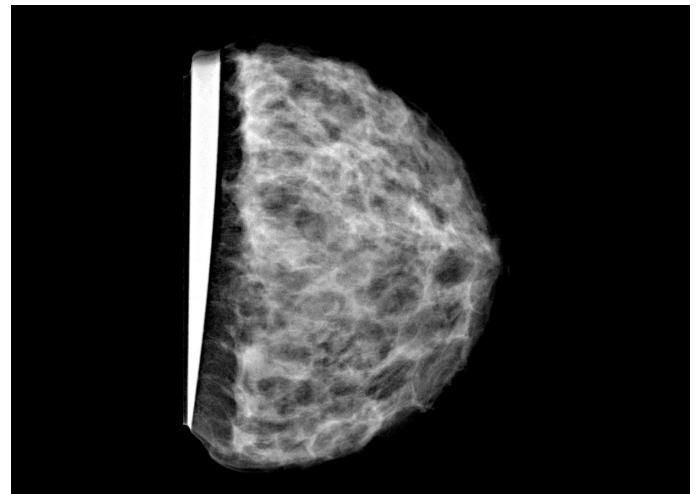

*Breast phantom.*

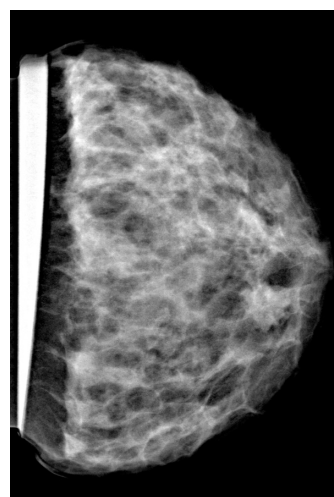


*Tumor slabs inserted.*

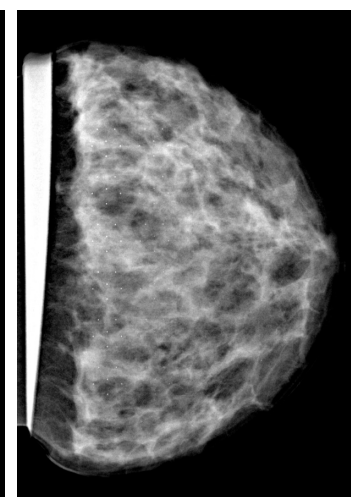


*Calcification pattern inserted.*


# BREAST PHANTOM

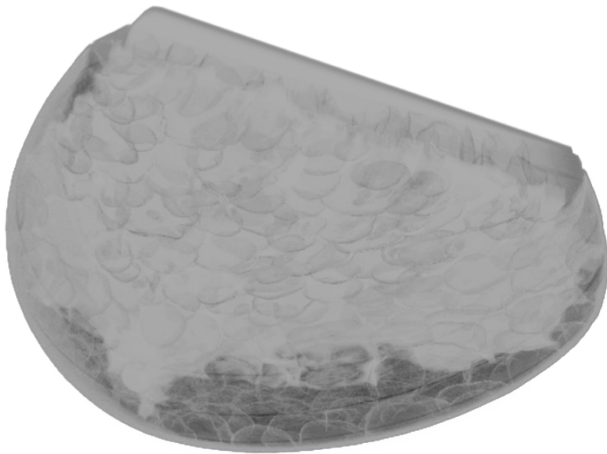


Phantom composed of 4 slabs simulating glandular and adipose tissue.

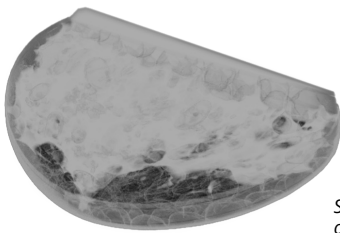

Section shows phantom composition of glandular and adipose tissue.

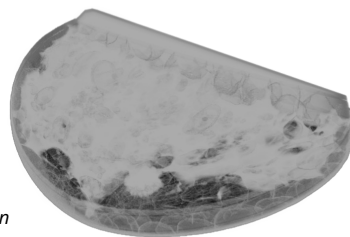

Section shows phantom composition after insertion of tumor slabs.

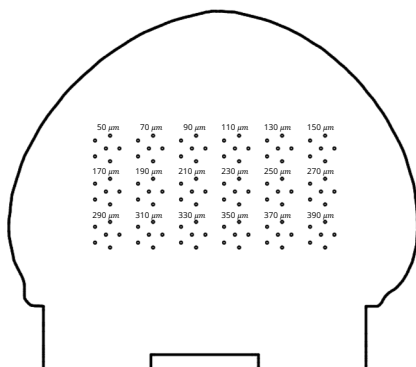

Drawing indicates diameter of microcalcifications of the insertable calcification pattern.

## Specifications

Size	Approx. 152 x 134 x 36 mm
Weight	Approx. 590 g
Components	4 slabs of 9 mm thickness
Positioning aid	Magnetic mount
Base material	Cellulose-polymer composite

## Diagnostic features

Realistic simulation of glandular and adipose tissue.

### Insertable calcification pattern

- Pattern thickness: 0.1 mm
- Calcification diameter: 0.05 to 0.39 mm

### Replacement slabs containing a spiculated mass

- Mass integrated in 2 additional slabs for replacement of the 2 central slabs
- Mass size: approx. 15 x 17 x 15 mm

For more information visit  
[www.phantomx.de](http://www.phantomx.de)

# BREAST PHANTOM


## General indications

- The phantom is made of a cellulose-polymer composite material with properties similar to hardwood. If handled carefully, it will last a long time.
- The phantom is coated with a protective layer. If the protective layer is undamaged, the phantom can be cleaned using a damp cloth (water or mild detergent).
- Protect from direct sunlight.
- Maintain a storage temperature of 10 °C to 30 °C. If the phantom is exposed to temperatures below -10 °C or above 45 °C, it can be severely damaged.
- The phantom is not equipped for dose measurements with dosimeters and it is not suited for tissue characterization by dual-energy contrast-enhanced mammography.
- The phantom is not certified as medical device.

## Attenuation properties


### Glandular Tissue

Linear attenuation coefficients [ $\text{cm}^{-1}$ ] (calculated)

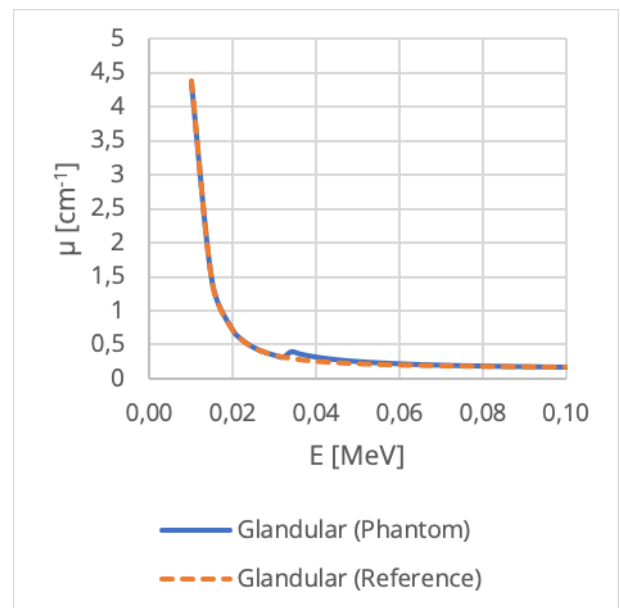

### Adipose Tissue

Linear attenuation coefficients [ $\text{cm}^{-1}$ ] (calculated)

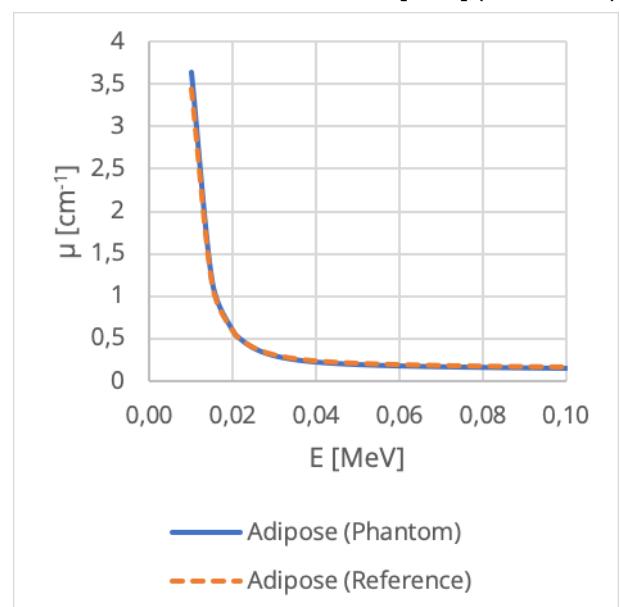

Phantom based on modified data, originally published by Ikejima LC, et al. Med Phys. 2017 and Graff CG. SPIE Medical Imaging: SPIE, 2016.

Tissue Reference: Woodard HQ, White DR. The composition of body tissues. Br J Radiol. 1986.