

FOOT PHANTOM METATARSAL FRACTURES

Age
Category

Adult

Body
Region

Extremities

Target
Modality

CT

Diagnostic
Features


Bone fractures



This phantom simulates a right foot with three non-displaced metatarsal fractures of metatarsale II, III and IV. It covers the entire foot including toes, metatarsus, tarsus and the distal parts of the tibia and fibula.

The phantom can be used in radiography and CT (including CBCT) and radiography to evaluate and optimize imaging performance and post-processing applications, including AI-enabled applications. It is also suited for training purposes.

The phantom provides a detailed and realistic simulation of soft and bone tissue.



FOOT PHANTOM METATARSAL FRACTURES




Specifications

Size	Approx. 95 x 245 x 100 mm
Weight	Approx. 780 g
Base material	Cellulose-polymer composite
Optimal tube voltage	120 kVp (cf page 3) - adaptable upon request -

Diagnostic features

Realistic simulation of bones and soft tissue.

Non-displaced fractures of the 2nd, 3rd and 4th metatarsal.

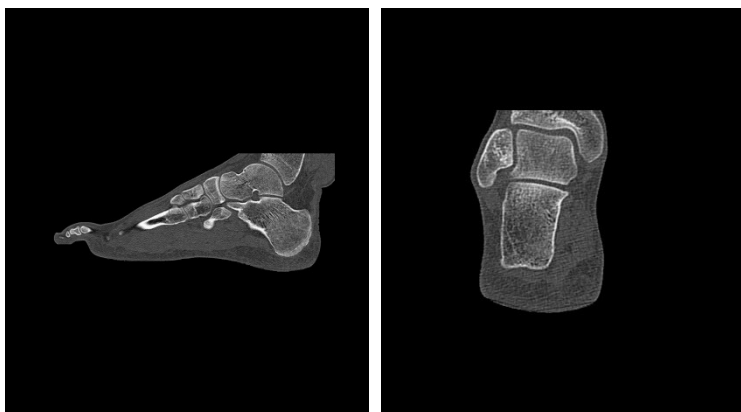

For more information visit
www.phantomx.de

FOOT PHANTOM METATARSAL FRACTURES


General indications

- The phantom is made of a cellulose-polymer composite material with properties similar to hardwood. If handled carefully, it will last a long time.
- The phantom is coated with a protective layer. If the protective layer is undamaged, the phantom can be cleaned using a damp cloth (water or mild detergent).
- Protect from direct sunlight.
- Maintain a storage temperature of 10 °C to 30 °C. If the phantom is exposed to temperatures below -10 °C or above 45 °C, it can be severely damaged.
- The phantom is not equipped for dose measurements with dosimeters and it is not suited for material characterization with dual energy CT.
- The phantom is not certified as medical device.
- Air voids are filled with cellulose-polymer composite of approx. -160 HU.


Attenuation properties

Soft Tissue

Linear attenuation coefficients [cm⁻¹] (calculated)




Hounsfield units (calculated)




Bone Tissue

Linear attenuation coefficients [cm⁻¹] (calculated)



Hounsfield units (calculated)



Tissue Reference: Woodard HQ, White DR. The composition of body tissues. Br J Radiol. 1986.